



# New West Dental Ceramics

2033 Swanson Ave. ■ Lake Havasu City, AZ 86403  
800-321-1614 ■ Fax 855-250-2830  
newwestlab.com

Dr. Name \_\_\_\_\_ Phone # \_\_\_\_\_

Acct. # \_\_\_\_\_ Patient Name/ID \_\_\_\_\_  
First Last

Address \_\_\_\_\_ Deliver by 5 p.m. on \_\_\_\_\_  
City/State/ZIP MM/DD/YR

Enclosed with case:  Impressions  Models  Bite  Photos  Other: \_\_\_\_\_


### ALL-CERAMIC & COMPOSITE

- BruxZir Full-Strength\* (> 1,000 MPa)
- NEW!** BruxZir Esthetic (> 900 MPa)  
(stump shade recommended for restorations less than 1.5 mm thick)
- IPS e.max \_\_\_\_\_ Stump Shade
- Composite

### PFM

- Obsidian Fused to Non-Precious\*
- Obsidian Fused to White Noble
- Obsidian Fused to White High Noble

### SHADE INSTRUCTIONS

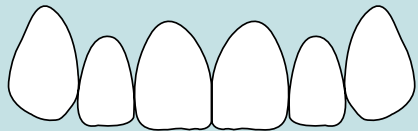


Final Shade \_\_\_\_\_ Indicate Shade Here

Stump Shade \_\_\_\_\_ Indicate Shade Here

Occlusal Staining:

- Light\*
- Med
- Dark
- None

### PONTIC DESIGN

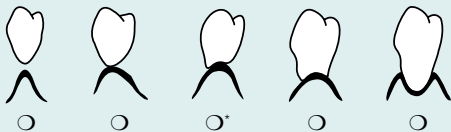

### SNORING & SLEEP APNEA DEVICES

- EMA
- TAP 3 TL
- dreamTAP
- Silent Nite


### MIGRAINE PREVENTION

- NTI-tss Plus
- NTI OmniSplint



### IF NO OCCLUSAL CLEARANCE

- Call doctor
- Spot opposing
- Metal occlusion
- Metal island
- Make this a permanent note in my master file

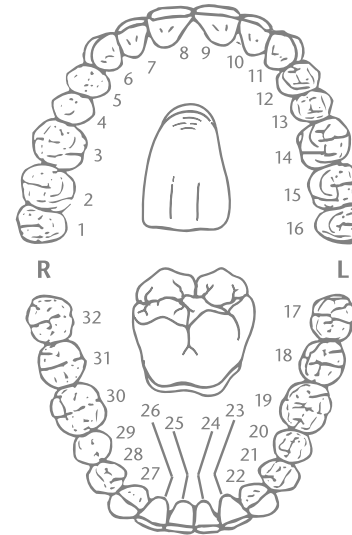

Signature \_\_\_\_\_  
Submission of this Rx constitutes agreement with limited warranty terms and conditions. See reverse for details.

License # \_\_\_\_\_ Date \_\_\_\_\_

### PROVISIONAL RESTORATIONS

- Transition Crowns & Bridges  
Abutment #(s) \_\_\_\_\_  
Pontic #(s) \_\_\_\_\_ Total units \_\_\_\_\_
- BioTemps Provisionals  
Reinforcement:  
 None  Wire\*  Fiber
- Splinted units\*  Individual units
- Perio treatment: Prepare tooth below gingival on tooth #(s) \_\_\_\_\_ by \_\_\_\_\_mm
- Cement-on implant
- Pontic site healing: Prepare ovate socket on tooth #(s) \_\_\_\_\_ by \_\_\_\_\_mm
- Screw-retained implant

### FULL-CAST

- Noble-Cast 60\*
- Noble-Cast 45
- Non-Precious

### CUSTOM ABUTMENTS

- Titanium\*
- Zirconia w/ Ti-Base
- Prepare existing abutment
- Implant System \_\_\_\_\_
- Diameter \_\_\_\_\_

*(See reverse for flat-rate pricing info)*

### BITE SPLINTS & NIGHTGUARDS

- Upper  Lower
- Comfort H/S (hard, with soft reline)\*
- Semi-hard EVA  Soft EVA
- Bleach tray
- CLEARsplint or day guard (self-adjusting, hard)
- Clear ortho retainer
- Essix retainer (one tooth)
- Clear-Lock Retainers  
 Set of 2  Set of 4  Set of 6

### PLAYSAFE MOUTHGUARDS

- Jr  Lt  Lt Pro
- Med  Hvy  Hvy Pro
- Helmet Strap
- (available in red or black)**
- Name \_\_\_\_\_

*Specify color(s) on Rx*

### VENEERS

- NEW!** BruxZir Esthetic
- IPS e.max  Layered IPS e.max

## TERMS AND WARRANTY INFORMATION



All Restorations Made in the USA

We honor VISA, MASTERCARD, AMEX and DISCOVER.

**TERMS:** Cost of collection of any account will be paid by the customer. All accounts are payable within 30 days of statement date. **Accounts not paid within the stated terms will be subject to COD status and a late charge of 2 percent of the unpaid balance.** Prices subject to change without notice. Rx must be enclosed with original case submission.

**NO-FAULT REMAKE POLICY:** New West is pleased to process all remakes or adjustments at no additional charge if requested within the warranty period and accompanied by the return of the original appliance.

**LIMITED WARRANTY/LIMITATION OF LIABILITY.** For warranty terms and conditions and limitation of liability, visit [newwestlab.com/warranty](http://newwestlab.com/warranty).



• BruxZir® Restorations



• Custom Abutments



- All-Ceramic Restorations
- PFM Restorations
- Full-Cast Restorations





• Mandibular Advancement Devices



- Nightguards
- Bite Splints
- Mouthguards

All rush cases must be prescheduled by calling 800-321-1614 before the case is shipped. Time of pickup and delivery may affect turnaround time.

## PREPARATION GUIDELINES

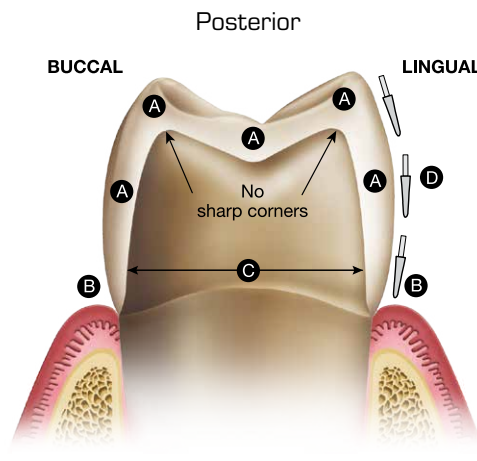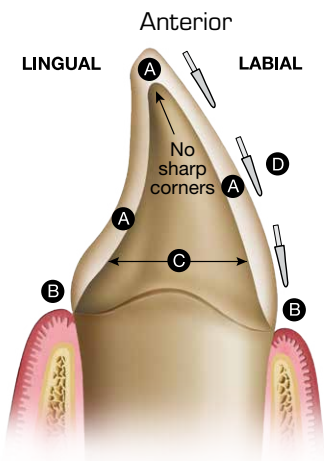

### BruxZir Esthetic

- A. 1.25 mm ideal reduction (0.7 mm minimum)
- B. Chamfer or modified shoulder margins preferred
- C. Axial walls must be convergent (avoid undercuts)
- D. Preparation should be cut in three planes
- E. To achieve optimal impression quality, gingival retraction is necessary for preparations with subgingival or equigingival margins

### BruxZir Full-Strength

- A. 1.0 mm ideal reduction (0.5 mm minimum)
- B. Chamfer or shoulder margins preferred. Feather-edge OK
- C. Axial walls must be convergent (avoid undercuts)
- D. Preparation should be cut in three planes
- E. To achieve optimal impression quality, gingival retraction is necessary for preparations with subgingival or equigingival margins

## FLAT-RATE PRICE ON CUSTOM ABUTMENTS AND SCREW-RETAINED CROWNS IS AVAILABLE FOR THE FOLLOWING IMPLANT SYSTEMS

BIOMET 3i™  
Certain®

CAMLOG®  
SCREW-LINE

DENTSPLY Implants  
ANKYLOS® C/X  
ASTRA TECH Implant System®  
ASTRA TECH Implant System® EV

Glidewell Direct  
Hahn™ Tapered Implant System  
Inclusive® Tapered Implant System

HIOSSEN®  
HG System

MegaGen  
AnyRidge® Implant System

Nobel Biocare  
Brånemark System® RP  
NobelActive®  
NobelReplace®

Straumann®  
Bone Level  
Tissue Level

Zimmer Dental  
Screw-Vent®

Restorations for the implant systems above are fabricated using components manufactured by Prismatic Dentalcraft, Inc. Prices may vary for other implant systems due to the need for original equipment manufacturer (OEM) components. Inclusive is a registered trademark of Prismatic Dentalcraft, Inc. Hahn Tapered Implant is a trademark of Prismatic Dentalcraft, Inc. All other trademarks are property of their respective owners.